BIOVIRIDIAN

Excellence in HPLC-MS Analysis

CERTIFICATE OF ANALYSIS

Web Verification Code: **COA11644**

SAMPLE RECEIVED
September 18, 2026

COA ISSUED
October 22, 2026

SAMPLE INFORMATION

Vendor
Certified Pep

Sample Name
J147, Dihexa, and Noopept 30mg

Sample Type
Capsule

Lot Number
J1dino-926F

Molecular Weight
350.3, 504.7, 318.4 g/mol


ANALYTICAL METHODS


Identity: Confirmed via LC–MS/MS
Purity: RP-HPLC (214 nm)
Content: HPLC quantitation

TEST RESULTS

Specification	Result	Method	Status
Identity: J147, Dihexa, and Noopept	J147, Dihexa, and Noopept	LC-MS/MS	✓ Conforms
Content	10.56, 11.41, 11.14 mg	HPLC Quantitation	✓ Conforms
Overall Purity	99.88%	RP-HPLC (214 nm)	✓ Conforms
Endotoxin	<0.05 EU/ml	<USP85>	✓ Conforms
Heavy Metals	<0.01 ppm	<USP232>	✓ Conforms

HPLC Chromatogram · Retention Time 9.583, 10.890, 11.324 **min**

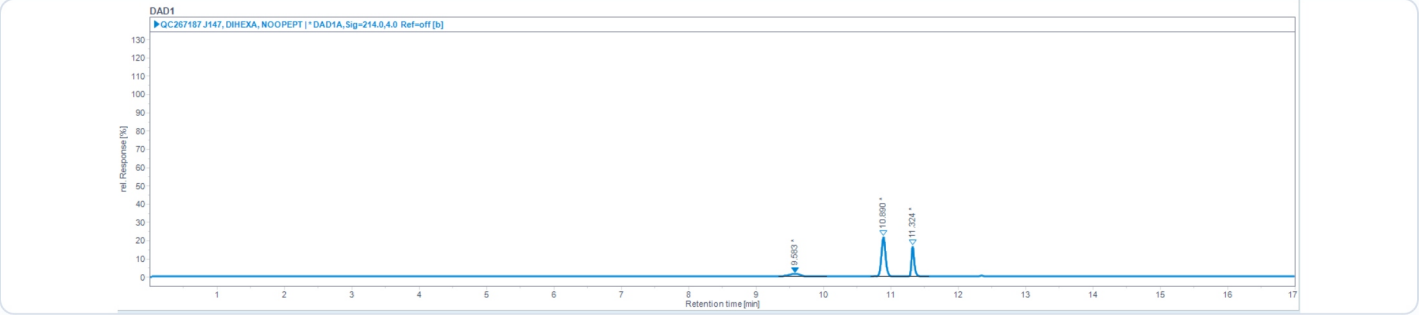

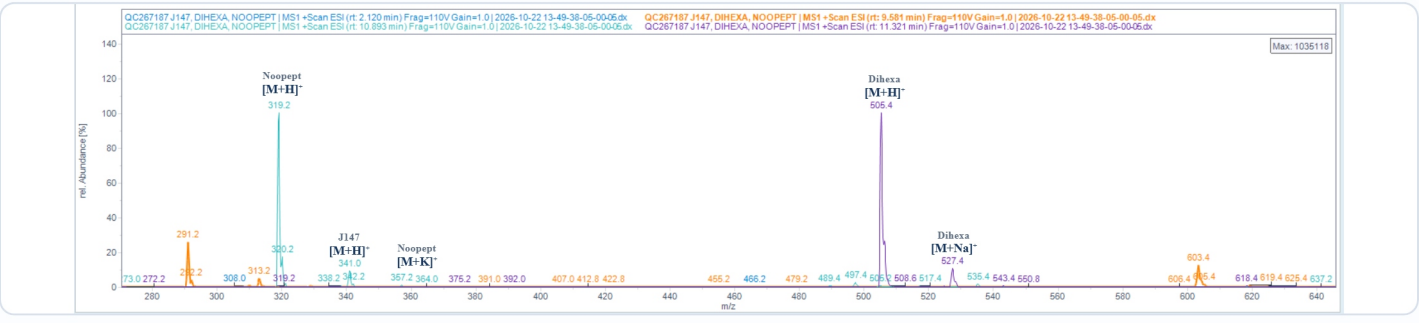

Certification: This Certificate of Analysis confirms that the tested material meets or exceeds Bioviridian's analytical quality specifications for peptide research use.

Verify authenticity at **bioviridians.com/coa-search.html** using the Web Verification Code above.

info@bioviridians.com

Shane Straight

Shane Straight, M.S.
Principal Chemist, Bioviridian Inc.