BIOVIRIDIAN

Excellence in HPLC-MS Analysis

CERTIFICATE OF ANALYSIS

Web Verification Code: **COA2796**

Sample Received: **January 30, 2026** COA Issued: **February 4, 2026**

PRODUCT INFORMATION

Vendor: **Cenexa Labs**

Sample Name: **Klow blend 80mg**

Sample Type: **Blue lyophilized powder**

Lot Number: **L2505-008**

MW: **1419, 4964, 343, & 403 g/mol**

ANALYTICAL METHODS


Identity: Confirmed via MALDI–MS
Purity: RP-HPLC (214 nm)
Content: HPLC quantitation


TEST RESULTS

Specification	Result	Method	Status
Identity: KLOW Blend	**BPC-157/TB-500/KPV/GHK-Cu**	**MALDI-MS**	✓ Conforms
Content	**9.87, 10.31, 11.34 and 51.43 mg**	HPLC Quantitation	✓ Conforms
Purity	**99.6%**	RP-HPLC (214 nm)	✓ Conforms


ANALYTICAL DATA


HPLC Chromatogram (Retention Time: 2.117, 2.408, 5.781, & 5.981 min)

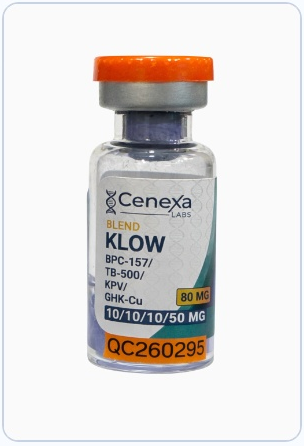

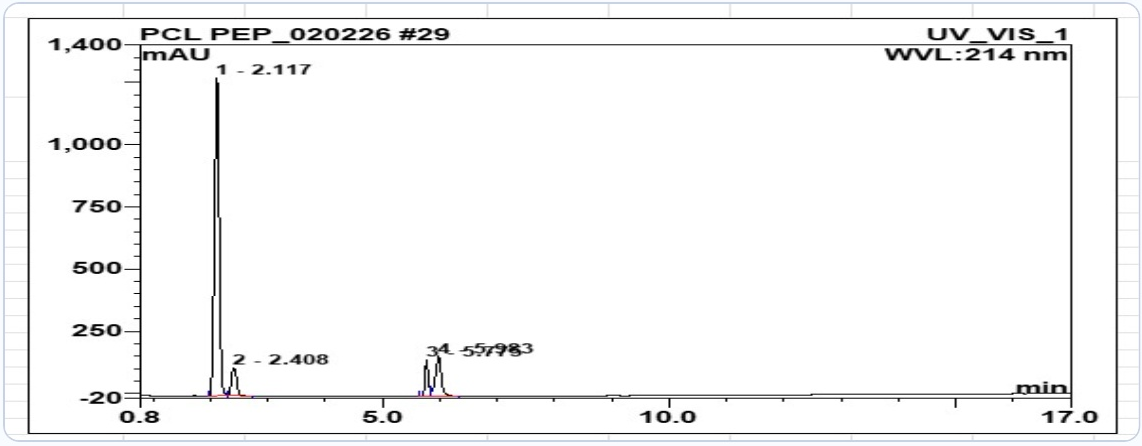

Mass Spectrum (MALDI-MS)

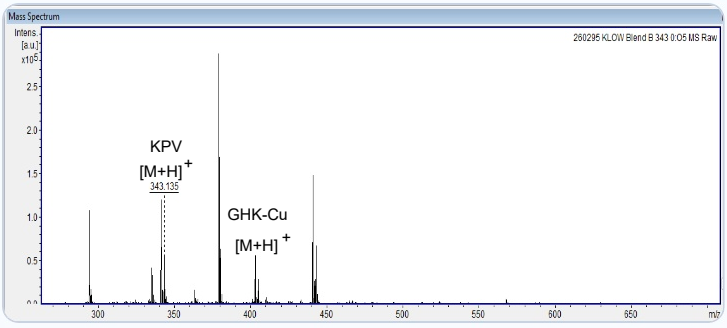

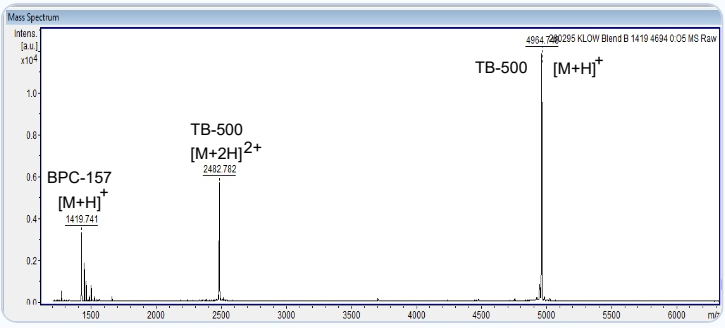

Certification: This COA confirms that the tested material meets or exceeds Bioviridian's analytical quality specifications for peptide research use.

Visit: https://bioviridians.com/coa-search.html

Shane Straight

Shane Straight, M.S.
Principal Chemist, Bioviridian Inc.

Contact: info@bioviridians.com