BIOVIRIDIAN

Excellence in HPLC-MS Analysis

CERTIFICATE OF ANALYSIS

Web Verification Code: **COA3569**

Sample Received: **April 1, 2026** COA Issued: **April 6, 2026**

PRODUCT INFORMATION

Vendor: **Peptides Source**

Sample Name: **Tesamorelin 20 mg**

Sample Type: **White lyophilized powder**

Lot Number: **NA**

MW: **5135.9 g/mol**

ANALYTICAL METHODS

Identity: Confirmed via MALDI–MS
Purity: RP-HPLC (214 nm)
Content: HPLC quantitation


TEST RESULTS

Specification	Result	Method	Status
Identity: Tesamorelin	**Tesamorelin**	**MALDI-MS**	✓ Conforms
Content	**21.25 mg**	HPLC Quantitation	✓ Conforms
Overall Purity	**99.8%**	RP-HPLC (214 nm)	✓ Conforms


ANALYTICAL DATA

HPLC Chromatogram (Retention Time: 7.950 min)



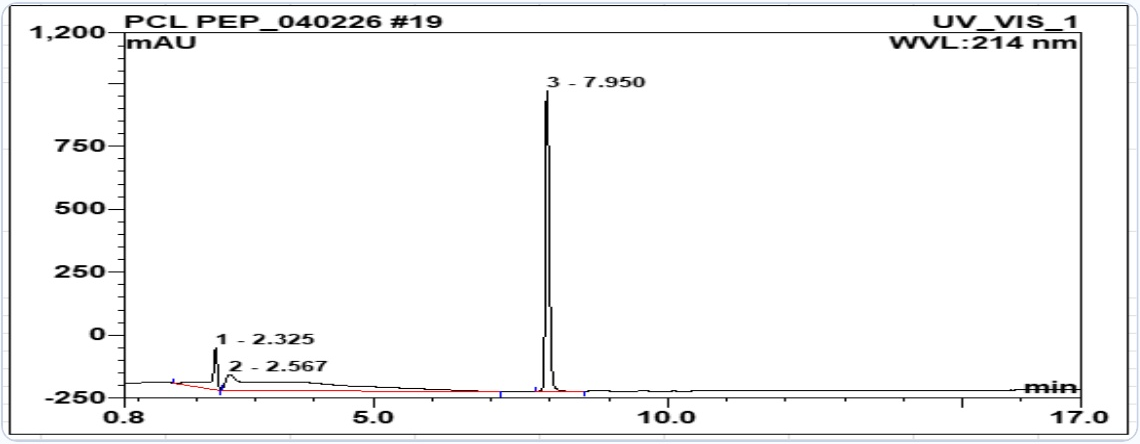

Mass Spectrum (MALDI-MS)

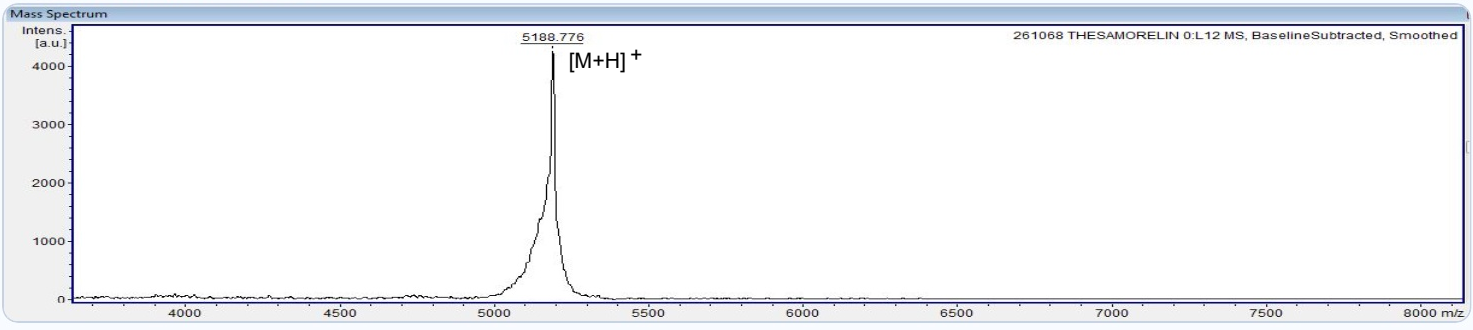

Certification: This COA confirms that the tested material meets or exceeds Bioviridian's analytical quality specifications for peptide research use.

Visit: https://bioviridians.com/coa-search.html

Shane Straight

Shane Straight, M.S.
Principal Chemist, Bioviridian Inc.

Contact: info@bioviridians.com