BIOVIRIDIAN

Excellence in HPLC-MS Analysis

CERTIFICATE OF ANALYSIS

Web Verification Code: **COA3943**

Sample Received: **April 22, 2026** COA Issued: **April 24, 2026**

PRODUCT INFORMATION

Vendor:	Sample Name:	Sample Type:	Lot Number:	MW:
Prime Peptides	**Klow Blend 80mg**	**Blue lyophilized powder**	**3182026KLO**	**1419.5, 4963.4, 342.1, 403.2 g/**

ANALYTICAL METHODS


Identity: Confirmed via MALDI–MS
Purity: RP-HPLC (214 nm)
Content: HPLC quantitation


TEST RESULTS


Specification	Result	Method	Status
Identity: BPC-157, TB-500, KPV, GHK-Cu	**BPC-157, TB-500, KPV, GHK-Cu**	**MALDI-MS**	✓ Conforms
Content	**10.76, 11.01, 10.14, 51.54 mg**	HPLC Quantitation	✓ Conforms
Overall Purity	**99.7%**	RP-HPLC (214 nm)	✓ Conforms

HPLC Chromatogram (Retention Time: 2.125, 2.442, 5.750, 6.075 **min)**



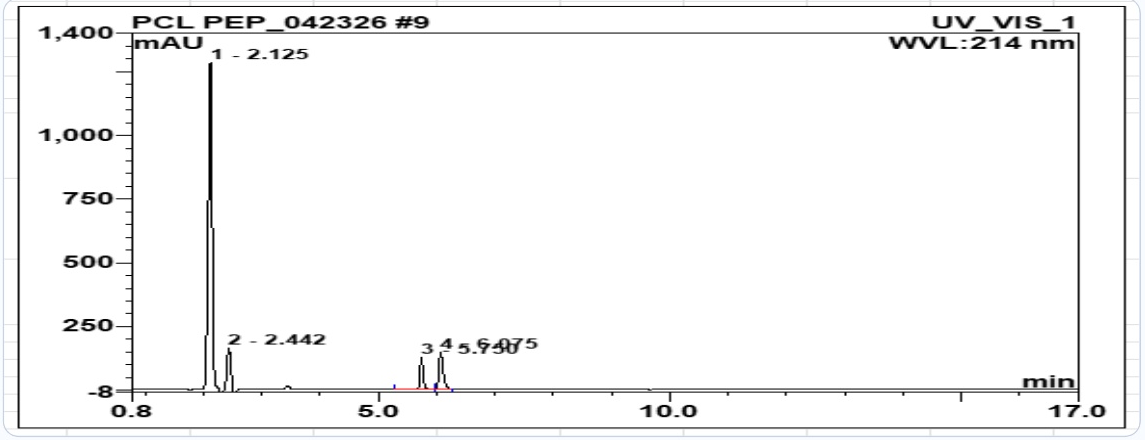

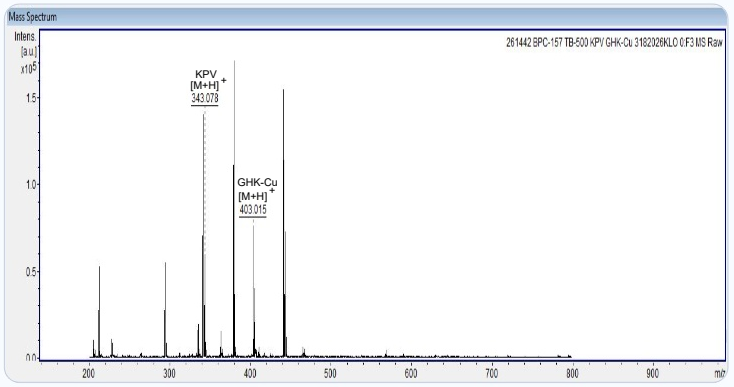

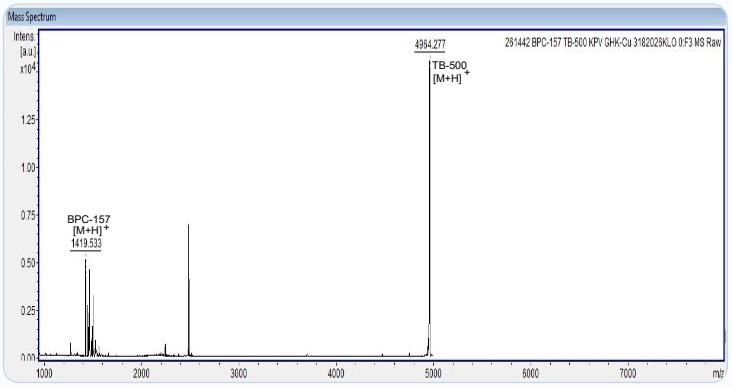

Certification: This COA confirms that the tested material meets or exceeds Bioviridian's analytical quality specifications for peptide research use.

Visit: https://bioviridians.com/coa-search.html

Shane Straight, M.S.
Principal Chemist, Bioviridian Inc.