

Sample Received: April 23, 2026

COA Issued: April 30, 2026

PRODUCT INFORMATION

|                      |              |                          |               |             |
|----------------------|--------------|--------------------------|---------------|-------------|
| Vendor:              | Sample Name: | Sample Type:             | Lot Number:   | MW (g/mol): |
| StrikePoint Peptides | Semax 5mg    | White lyophilized powder | XA-202604-001 | 813.9       |



ANALYTICAL METHODS

Identity: Confirmed via MALDI-MS  
Purity: RP-HPLC (214 nm)  
Content: HPLC quantitation

TEST RESULTS

| Specification   | Result  | Method            | Status     |
|-----------------|---------|-------------------|------------|
| Identity: Semax | Semax   | MALDI-MS          | ✓ Conforms |
| Content         | 5.39 mg | HPLC Quantitation | ✓ Conforms |
| Overall Purity  | 99.8%   | RP-HPLC (214 nm)  | ✓ Conforms |

HPLC Chromatogram (Retention Time: 6.233 min)

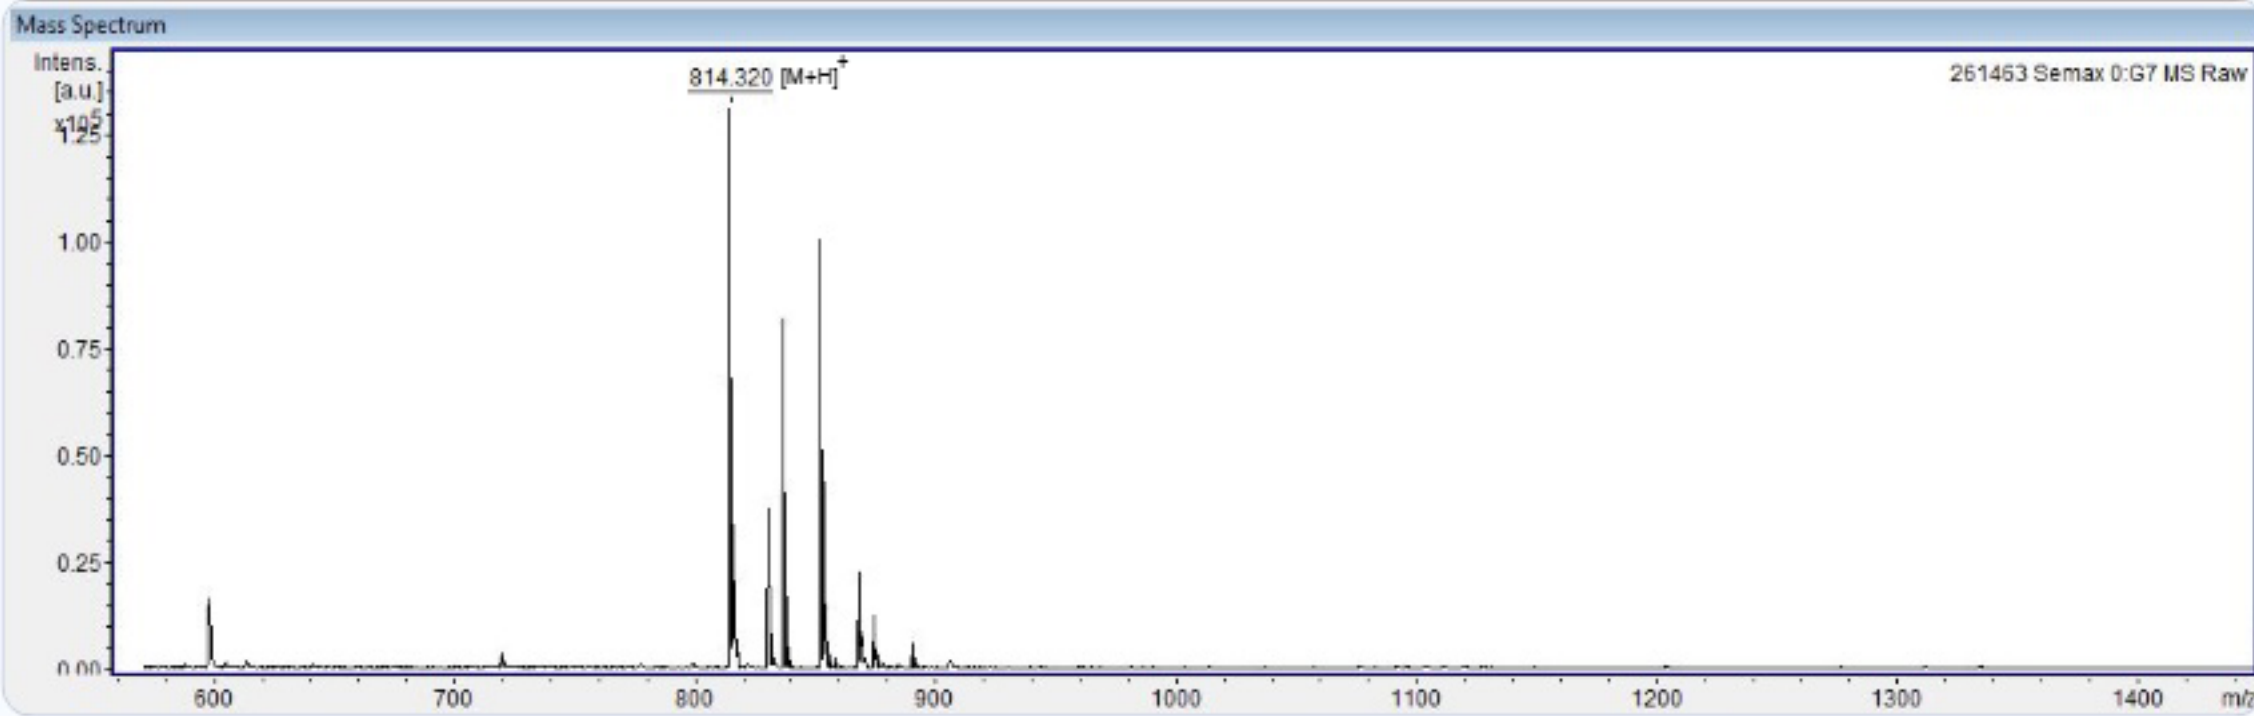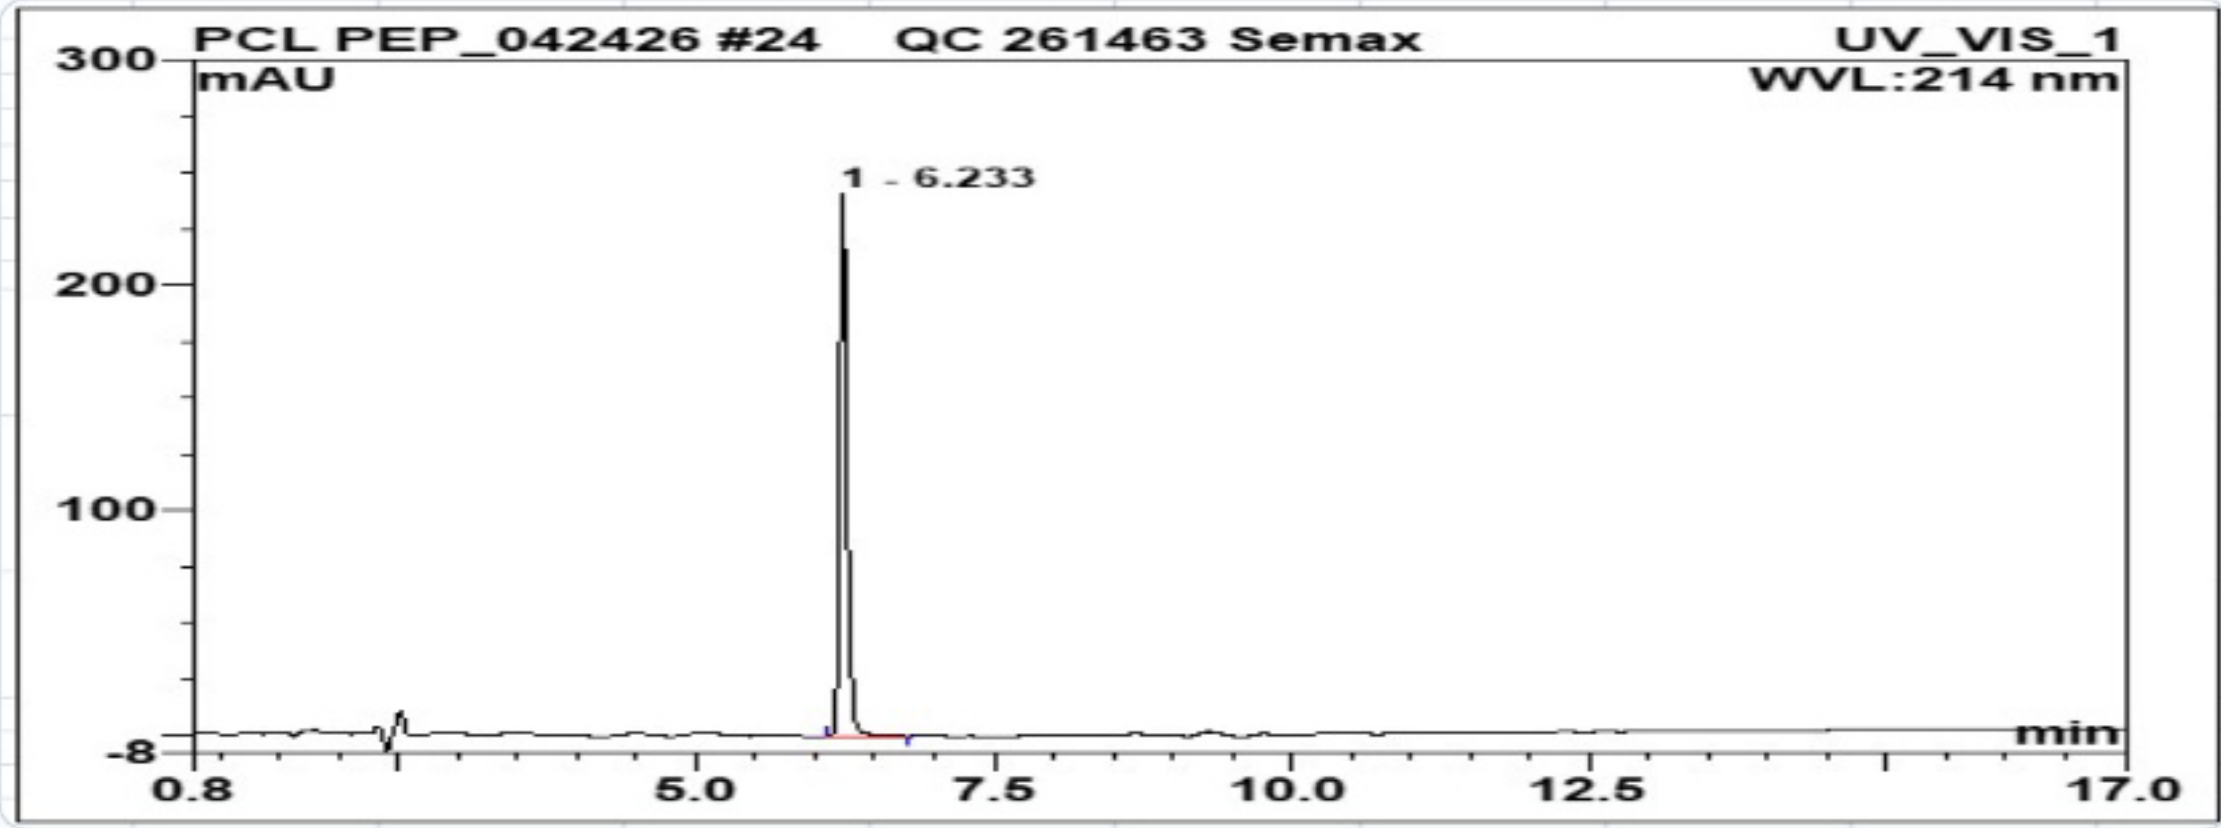

Certification: This COA confirms that the tested material meets or exceeds Bioviridian’s analytical quality specifications for peptide research use.  
Visit: <https://bioviridians.com/coa-search.html>



Shane Straight

Shane Straight, M.S.  
Principal Chemist, Bioviridian Inc.