

Sample Received: May 6, 2026
COA Issued: June 17, 2026

PRODUCT INFORMATION


Table with 5 columns: Vendor, Sample Name, Sample Type, Lot Number, MW (g/mol). Values: Cell Syntax, BAC Water, Clear liquid, CD013026A, 91.0.

ANALYTICAL METHODS

Identity: Confirmed via MALDI-MS
Purity: RP-HPLC (214 nm)
Content: HPLC quantitation

TEST RESULTS

Table with 4 columns: Specification, Result, Method, Status. Rows include Identity (BAC Water, Benzyl Alcohol, MALDI-MS, Conforms), Content (0.998 %, HPLC Quantitation, Conforms), Overall Purity (99.9%, RP-HPLC (214 nm), Conforms), and pH (6.90, pH Meter, Conforms).

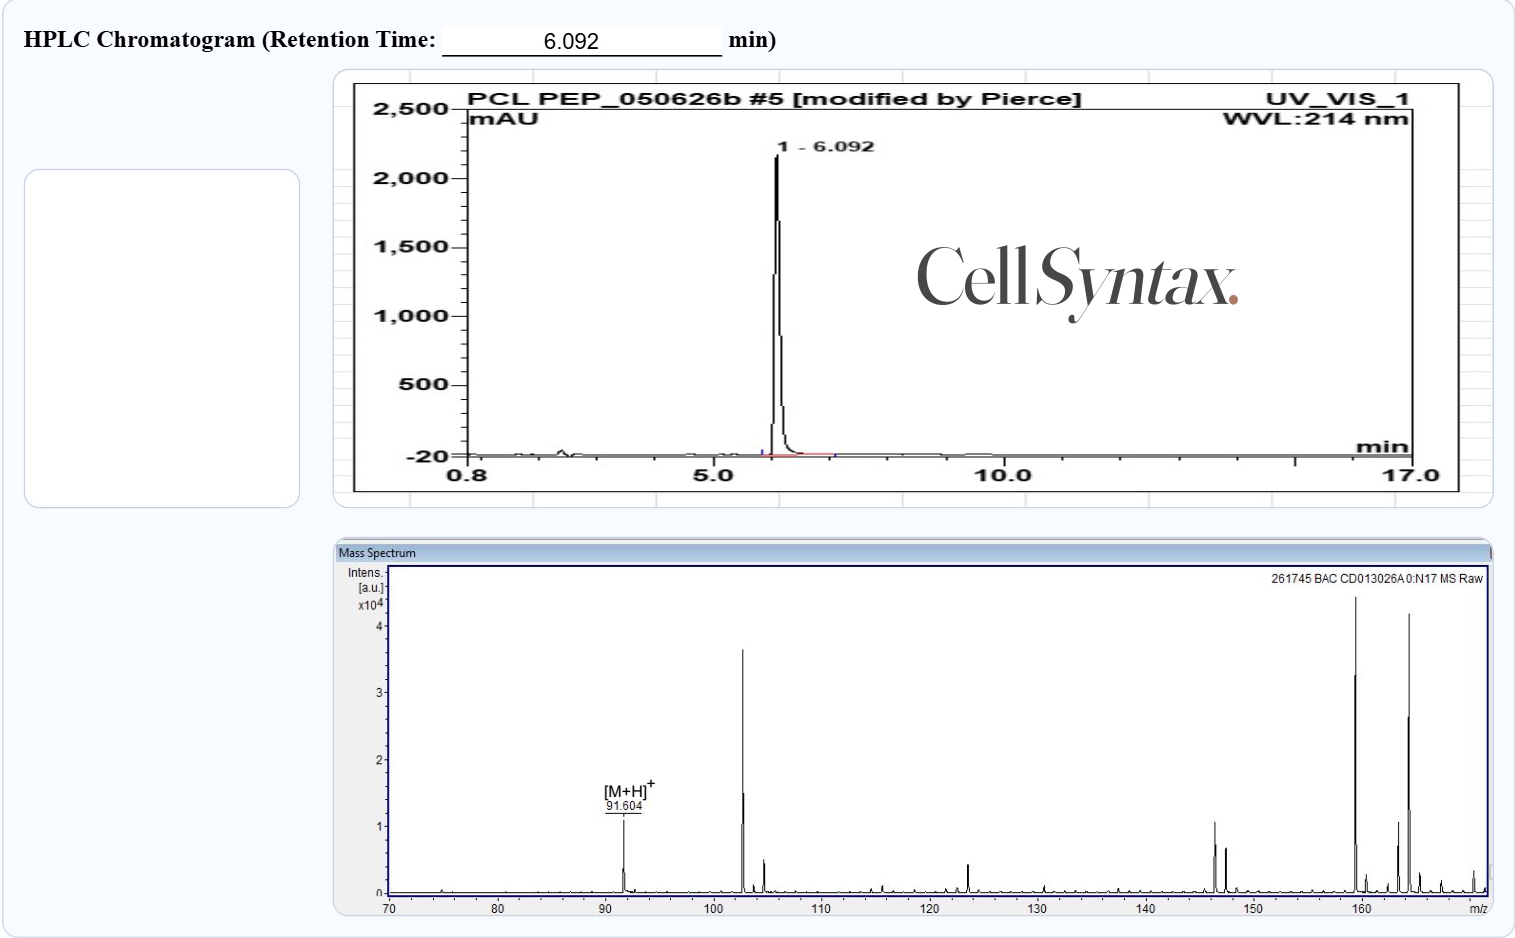

Certification: This COA confirms that the tested material meets or exceeds Bioviridian’s analytical quality specifications for peptide research use.
Visit: https://bioviridians.com/coa-search.html
Shane Straight, M.S.
Principal Chemist, Bioviridian Inc.

