BIOVIRIDIAN

Excellence in HPLC-MS Analysis

CERTIFICATE OF ANALYSIS

Web Verification Code: **COA7221**

SAMPLE RECEIVED
August 3, 2026

COA ISSUED
August 12, 2026

SAMPLE INFORMATION

Vendor
PeakForce Labs

Sample Name
BAC Water 30mL

Sample Type
Clear liquid

Lot Number
BAW30-0726-A

MW (g/mol)
91.1

ANALYTICAL METHODS


Identity: Confirmed via LC–MS/MS
Purity: RP-HPLC (214 nm)
Content: HPLC quantitation


TEST RESULTS

Specification	Result	Method	Status
Identity: BAC Water	Benzyl Alcohol	LC-MS/MS	✓ Conforms
Content	1.002 %	HPLC Quantitation	✓ Conforms
Overall Purity	99.81%	RP-HPLC (214 nm)	✓ Conforms
pH	9.38	<pH Meter>	✓ Conforms

HPLC Chromatogram · Retention Time 5.757 **min**



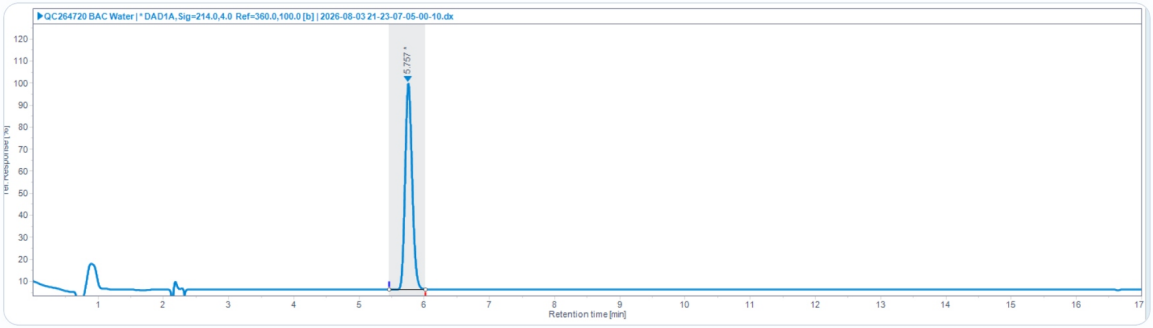

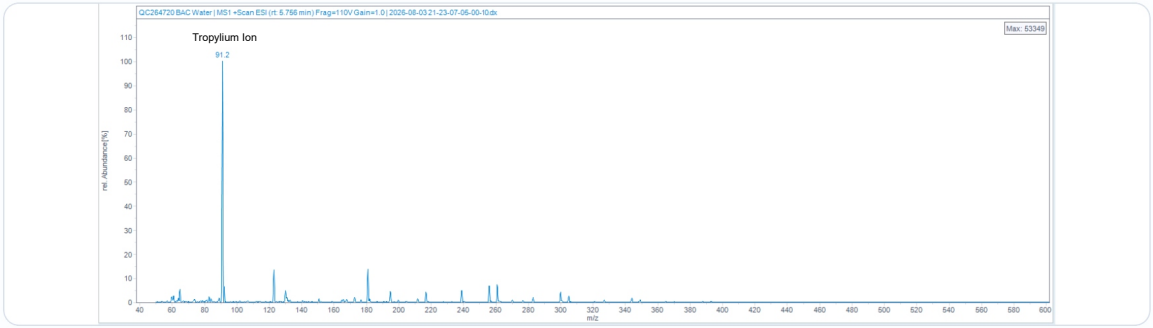

Certification: This Certificate of Analysis confirms that the tested material meets or exceeds Bioviridian's analytical quality specifications for peptide research use.

Verify authenticity at **bioviridians.com/coa-search.html** using the Web Verification Code above.

info@bioviridians.com

Shane Straight

Shane Straight, M.S.
Principal Chemist, Bioviridian Inc.